

Model KBF 115 | Constant climate chambers with large temperature / humidity range

The BINDER KBF is the specialist for unconditionally reliable stability testing and precise maintenance of constant climate conditions. From programming to documentation, this constant climate chamber meets all critical requirements.

BENEFITS

- Homogeneous climate conditions thanks to APT.line™ technology
- Automatic water and wastewater management
- Pressure humidification with fast response times



Model 115

MAIN FEATURES

- Temperature range: 0 °C to 70 °C
- Humidity range: 10 % to 80 % RH
- APT.line™ preheating chamber technology
- Humidity regulation with capacitive humidity sensor and vapor humidification
- Intuitive touchscreen controller with time-segment and real-time programming
- Internal data logger, measured values can be read out in open format via USB
- Unit self-test for comprehensive status analysis
- Tight-sealing inner door made of safety glass (ESG)
- Avoidance of glass corrosion by special TIMELESS coating
- Inner chamber made of stainless steel
- 2 stainless steel racks
- Access port with silicone plug, 30 mm, left
- Class 3.1 independent temperature safety device (DIN 12880) with visual and audible temperature alarm
- Computer interface: Ethernet
- Door heating

ORDERING INFORMATION


| Interior volume [L] | Voltage | Option model | Version | Art.-No. |
|---------------------|----------------------------|--------------|---------------|-----------|
| Model KBF 115 | | | | |
| 102 | 200...230 V 1~ ph 50/60 Hz | Standard | KBF115-230V | 9020-0320 |
| | 200...240 V 1~ ph 50/60 Hz | Standard | KBF115UL-240V | 9020-0321 |

TECHNICAL DATA


| Description | KBF115-230V ¹ | KBF115UL-240V ¹ |
|------------------------------------------------------------------------|--------------------------|----------------------------|
| Article Number | 9020-0320 | 9020-0321 |
| Performance Data Temperature | | |
| Temperature range [°C] | 0...70 | 0...70 |
| Temperature variation at 40 °C [± K] | 0.2 | 0.2 |
| Temperature fluctuation [± K] | 0.1 | 0.1 |
| Max. heat compensation at 40 °C [W] | 200 | 200 |
| Performance Data Climate | | |
| Temperature range [°C] | 10...70 | 10...70 |
| Temperature variation at 25 °C and 60 % RH [± K] | 0.2 | 0.2 |
| Temperature variation at 40 °C and 75 % RH [± K] | 0.2 | 0.2 |
| Temperature fluctuation at 25 °C and 60 % RH [± K] | 0.1 | 0.1 |
| Temperature fluctuation at 40 °C and 75 % RH [± K] | 0.1 | 0.1 |
| Humidity range [% RH] | 10...80 | 10...80 |
| Humidity fluctuation at 25 °C and 60 % RH | ≤2 ± % RH | ≤2 ± % RH |
| Humidity fluctuation at 40 °C and 75 % RH | ≤2 ± % RH | ≤2 ± % RH |
| Humidity recovery time after 30 s door open at 25 °C and 60 % RH [min] | 6 | 6 |
| Humidity recovery time after 30 s door open at 40 °C and 75 % RH [min] | 7 | 7 |
| Electrical data | | |
| Rated Voltage [V] | 200...230 | 200...240 |
| Power frequency [Hz] | 50/60 | 50/60 |
| Nominal power [kW] | 0 | 0 |
| Unit fuse [A] | 16 | 16 |
| Phase (Nominal voltage) | 1~ | 1~ |
| Internal Dimensions | | |
| Depth [mm] | 351 | 351 |
| Height [mm] | 483 | 483 |
| Width [mm] | 600 | 600 |
| Housing dimensions not incl. fittings and connections | | |
| Width net [mm] | 880 | 880 |
| Height net [mm] | 1050 | 1050 |
| Depth net [mm] | 650 | 650 |
| Measures | | |
| Wall clearance back [mm] | 100 | 100 |
| Wall clearance sidewise [mm] | 100 | 100 |
| Interior volume [L] | 102 | 102 |
| Net weight of the unit (empty) [kg] | 128 | 128 |
| permitted load [kg] | 100 | 100 |
| Load per rack [kg] | 30 | 30 |
| Doors | | |
| Inner doors | 1 | 1 |
| Unit doors | 1 | 1 |
| Environment-specific data | | |
| Energy consumption at 40 °C and 75 % RH [Wh/h] | 470 | 470 |
| Sound-pressure level [dB(A)] | 52 | 52 |
| Fixtures | | |
| Number of shelves (std./max.) | 2/5 | 2/5 |

¹ All technical data is specified for unloaded units with standard equipment at an ambient temperature of +22 °C ±3 °C and a power supply voltage fluctuation of ±10 %. The temperature data is determined in accordance to BINDER factory standard following DIN 12880, observing the recommended wall clearances of 10 % of the height, width, and depth of the inner chamber. Technical data refers to 100 % fan speed. All indications are average values, typical for units produced in series. We reserve the right to change technical specifications at any time.

DIMENSIONS incl. fittings and connections [mm]

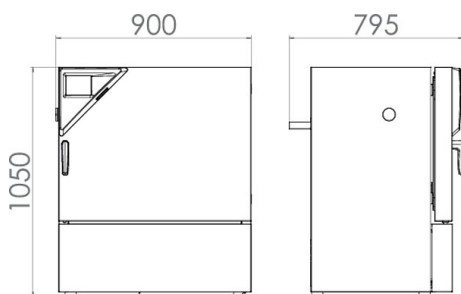


CHARTS

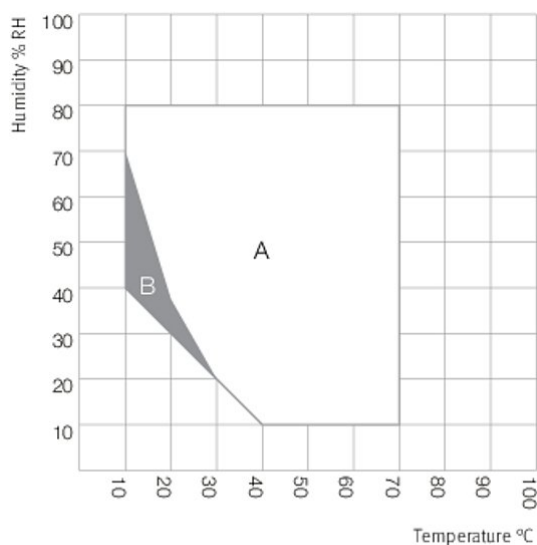

A: Guaranteed condensation-free range
B: Time-limited operation (max. 24 hours)

Climate chart

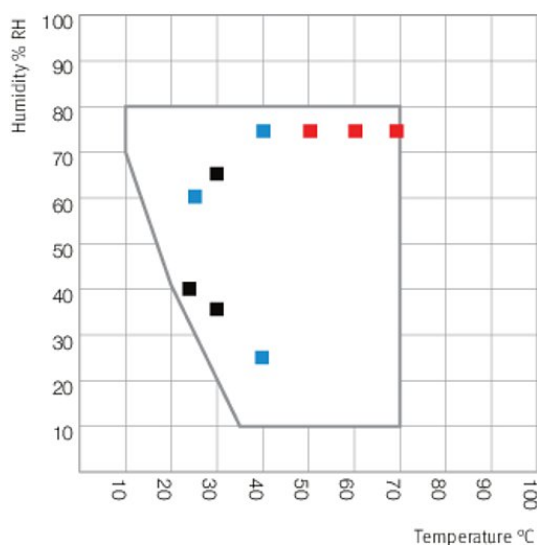

■ Long term testing (ICH Q1A)
■ Accelerated testing (ICH Q1A)
■ Stress testing (ICH Q1A)

Temperature-humidity chart with ICH checkpoints

OPTIONS AND ACCESSORIES

| Designation | Description | * | Art.-No. |
|--------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|----|-----------|
| Access port with silicone plug | left | | |
| | 30 mm | 01 | 8012-1442 |
| | 50 mm | 01 | 8012-1472 |
| | 100 mm | 01 | 8012-0515 |
| | right | | |
| | 30 mm | 01 | 8012-1436 |
| | 50 mm | 01 | 8012-1466 |
| | 100 mm | 01 | 8012-0514 |
| | top | | |
| | 30 mm | 01 | 8012-1448 |
| | 50 mm | 01 | 8012-1454 |
| | 100 mm | 01 | 8012-1460 |
| Alarm output, zero-voltage | for temperature (± 2 °C) and humidity (± 5 % RH), accessible via 6-pin DIN socket (max. 24 V - 2.5 A), with audible signal that can be switched off | – | 8012-1036 |
| Analog output 4-20 mA | for temperature and humidity values (output not adjustable) | – | 8012-1039 |
| APT-COM™ 4 BASIC-Edition | for simple logging and documentation requirements with up to 5 networked units. version 4, BASIC edition | 19 | 9053-0039 |

* Notes › See last page

| Designation | Description | * | Art.-No. |
|---------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----|-----------|
| APT-COM™ 4 GLP-Edition | for working under GLP-compliant conditions. Measured values are documented in a tamper-proof way in line with the requirements of FDA Regulation 21 CFR 11. version 4, GLP edition | 19 | 9053-0042 |
| APT-COM™ 4 PROFESSIONAL-Edition | convenient unit and user management built on the BASIC edition. Suitable for networking up to 100 units. version 4, PROFESSIONAL edition | 19 | 9053-0040 |
| BINDER PURE AQUA SERVICE | system for preparation or complete desalination of tap water, containing single-use cartridge, hoses and measuring device | – | 8012-0759 |
| BINDER PURE AQUA SERVICE, accessories | Single-use, replacement cartridge for BINDER PURE AQUA System | – | 6011-0165 |
| Calibration certificate, expanded | for temperature and humidity; for extending the measurement in center of chamber to include another test value | – | 8012-0155 |
| Calibration certificate, temperature | temperature measurement incl. certificate and 27 measuring points at specified temperature | – | 8012-0923 |
| | temperature measurement incl. certificate, 15- 18 measuring points at specified temperature | – | 8012-0920 |
| | temperature measurement incl. certificate, 9 measuring points at specified temperature | – | 8012-0917 |
| Calibration certificate, temperature and humidity | Measurement in center of chamber at 25 °C / 60% RH or at specified test values | – | 8012-0154 |
| | temperature (according to DIN12880) and humidity measurement incl. certificate, 27 temperature measuring points and 1 humidity measuring point, at 25 °C / 60 % RH or at specified values | – | 8012-0924 |
| Class 3.3 independent temperature safety device | with visual alarm (DIN 12880) | – | 8012-1032 |
| Converter, voltage | to operate the device at a nominal voltage of 120 V 1 ph 60 Hz 240 V option model | – | 8009-0821 |
| Data Logger Kit | T 220: For continuous temperature logging from -90 °C to 220 °C. The kit includes 1 data logger, Pt 100 sensor with 2 m extension cable and 1 magnetic fixture for mounting to the BINDER unit | 19 | 8012-0715 |
| | TH 70/70: For continuous temperature and humidity logging from -40 °C to 70 °C / 0% to 100% RH and additional logging of ambient conditions. Kit includes 1 data logger, 2 attachable combined humidity/temperature sensors, 2 m extension cable and 1 fixture for mounting to the BINDER unit | 19 | 8012-0717 |
| | TH 70: For continuous temperature and humidity logging from -40 °C to 70 °C; 0% to 100% RH. Kit includes 1 data logger, Pt 100 sensor with 2 m extension cable, and 1 magnetic fixture for mounting to the BINDER unit | 19 | 8012-0716 |
| Data Logger Software | LOG ANALYZE software kit, configuration and evaluation software for all BINDER Data Logger Kits (incl. USB data cable) | 19 | 8012-0821 |
| Door lock | lockable door handle | – | 8012-1023 |
| Interior socket | Waterproof, switched flush-mounting box (CA3GD) for nominal voltage in unit interior, with cover and corresponding plug (nominal voltage; max. 500 W; max. 90 °C; protection class IP67) | 07 | 8012-1043 |
| LED light bars | Basic set consisting of 2 pieces, attachment material, control unit for max. 4 light strips, 100-240 V, 50/60 Hz | | |
| | Basic set 300, length 30 cm | – | 8012-1107 |
| | Basic set 500, length 50 cm | – | 8012-1108 |
| | Expansion set consisting of 2 pieces, attachment material: clips. For expanding the basic set of light bars | | |
| | Expansion set 300, length 30 cm | – | 8012-1716 |
| | Expansion set 500, length 50 cm | – | 8012-1717 |
| pH-neutral detergent | concentrated, for gentle remove of residual contaminants; 1 kg | – | 1002-0016 |
| Pt 100 temperature sensor | additional flexible Pt 100, interior, for displaying the temperature on the unit display | – | 8012-1042 |
| Rack | stainless steel | – | 6004-0112 |
| Rack accessories | fasteners (1 set of 4) for additional security of racks | – | 8012-0620 |
| Rack, reinforced | stainless steel, with fasteners (1 set of 4) | – | 8012-0700 |
| RS 485 / RS 422 interface converter | RS 422 cable set and RS 485 / RS 422 interface converter for connection to 10-way plug distributor | | |
| | 115 V option model | – | 8012-0599 |
| | 230 V option model | – | 8012-0589 |
| RS 485 interface, 2-wire | Additional serial interface can be used parallel to Ethernet, for Multi Management Software APT-COM™ | – | 8012-1066 |
| Shelf, perforated | Stainless steel | – | 6004-0115 |
| Water supply set | consisting of fresh- and waste-water containers (20 liters each), cabling and pump | | |
| | external, free-standing | – | 8012-1846 |
| | external, consisting of fresh- and waste-water containers (20 liters each), cabling and pump | | |
| | external, for hanging from the back of the device | – | 8012-0643 |

* Notes › See last page

SERVICES

| Designation | Description | * | Art.-No. |
|----------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------|-----------|
| Installation services | | | |
| Installation | and set up of unit at operating location, connect to existing connections | 13, 18 | DL10-0300 |
| Instruction | unit function instructions for operation and programming of the controller | 18 | DL10-0700 |
| Preventive maintenance | | | |
| Preventive maintenance | Executive of equipment inspection according to maintenance plan | 14, 18 | DL20-0400 |
| Calibration services | | | |
| Calibration temperature and humidity | including certificate, one measuring point in center of chamber at 25 °C / 60 % RH or at specified values | 14, 16, 17, 18 | DL30-0301 |
| Temperature and humidity measurement according to DIN12880 | including certificate (27 temperature measuring points and one humidity measuring point, at 25 °C / 60 % RH or at specified values) | 14, 16, 17, 18 | DL30-0427 |
| Temperature measurement 18 temperature measuring points and 1 humidity measuring point | including certificate, 18 temperature measuring points and 1 humidity measuring point in center of chamber, at 25 °C / 60 % RH or at specified values | 14, 16, 17, 18 | DL30-0318 |
| Temperature measurement 27 temperature measuring points and 1 humidity measuring point | including certificate, 27 temperature measuring points and 1 humidity measuring point in center of chamber, at 25 °C / 60 % RH or at specified values | 14, 16, 17, 18 | DL30-0327 |
| Temperature measurement 9 temperature measuring points and 1 humidity measuring point | including certificate, 9 temperature measuring points and 1 humidity measuring point in center of chamber, at 25 °C / 60 % RH or at specified values | 14, 16, 17, 18 | DL30-0309 |
| Validation services | | | |
| Execution of IQ/OQ | in accordance with qualification folder | 15, 18, 20 | DL42-0300 |
| Execution of IQ/OQ/PQ | in accordance with customer's requirement, price: on request | 15, 18 | DL44-0500 |
| Qualification folder IQ/OQ | supporting documents for validation performed by customer, consisting of: IQ/OQ checklists, unit schematics, QM certificate in accordance with ISO 9001 | 15, 18, 20 | 8012-0867 |
| Qualification folder IQ/OQ/PQ | supporting documents for validation performed by customer, in accordance with customer's requirement, extension of Qualification folder IQ/OQ by chapter PQ | 15, 18 | 8012-0955 |
| Warranty service | | | |
| Extension of the warranty from 2 to 3 years | beginning with the date of delivery, wearing parts are not included | – | DL01-4041 |
| Extension of the warranty from 2 to 5 years | beginning with the date of delivery, wearing parts are not included | – | DL01-4042 |

* Notes › See last page



Wolf Laboratories Limited

www.wolflabs.co.uk

Tel: 01759 301142

Fax: 01759 301143

sales@wolflabs.co.uk



Use the above details to contact us if this literature doesn't answer all your questions.

Pricing on any accessories shown can be found by keying the part number into the search box on our website.

The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed to be correct. If there are aspects of the specification that must be guaranteed, please provide these to our sales team so that details can be confirmed.

