

# Frozen in Time Ltd

Manufacturers of Freeze Drying Machines and Vacuum Cold traps

## Operating Manual **F100**



**Operating Manual**

**F100 freeze driers**

Order Number:

Serial Number:

In case of enquiries please state the above

For service please contact:

**FROZEN IN TIME**<sup>LTD</sup>  
York Road Industrial Park, Sheriff Hutton  
York, YO60 6RZ, England  
[info@freezedriers.com](mailto:info@freezedriers.com)

**Telephone:** 01347 878158  
**International:** +44 1347 878158

# Contents

<b>1. General Information</b>	
1.1. Introduction .....	5
1.2. <b>100KG</b> freeze drier technical data.....	6
1.3. Safety instructions.....	7
1.3.1. Disconnect the mains plug.....	7
1.3.2. Solvents.....	7
1.3.3. Cleaning and Maintenance.....	7
1.3.4. Danger of freezing skin to cold surfaces.....	7
1.4. The <b>100KG</b> freeze driers should not be used when.....	8
<b>2. Description of the Freeze Drying Processes</b>	
2.1. General Information on Freeze Drying .....	9
2.2. Freezing the product.....	12
2.3. Primary drying.....	12
2.4. Secondary drying.....	14
2.5. Air admittance.....	15
2.6. Defrosting .....	15
<b>3. Installation and Commissioning of the Unit</b>	
3.1. Site of installation.....	16
3.2. Mains power.....	16
3.3. Air Admittance.....	16
3.4. Drain valve for condensate.....	16
3.5. Vacuum pump exhaust gases.....	16
<b>4. Operating the 100KG Freeze Driers</b>	
4.1 Loading Trays .....	17
4.2. Vacuum Pump.....	18
4.3. Condenser drain valve.....	19
4.4. Circuit breakers.....	19
<b>5. The control system</b>	
5.1. Main Control Screen.....	21
5.2. Overview Screen.....	22
5.3. Recipe Screen.....	23
5.4. Graph.....	28
5.5. Engineering.....	31
<b>6. Reporting.....</b>	<b>36</b>

## **7. Troubleshooting**

7.1. Power failure .....	37
7.2. Insufficient vacuum .....	37
7.3. Insufficient cooling of the condenser chamber.....	38
7.4. Insufficient defrosting of the condenser chamber.....	38
7.5. Insufficient cooling of the shelves.....	38
7.6. Insufficient heating of the shelves.....	38
7.7. Fluctuations in shelf temperatures .....	39
7.8. Defrost will not drain.....	39
7.9. Air admittance will not open.....	39
6.10. Doors will not seal under vacuum.....	39
6.11. Incorrect probe temperature.....	39

## **8. Maintenance**

8.1. Ice condenser chamber .....	40
8.2. Heat exchanger.....	40
8.3. Rubber seals .....	40
8.4. Vacuum pump.....	40
8.5. Exhaust filter .....	40
8.6. Cleaning.....	40
8.7. Checks by the operator .....	41

# 1. General Information

## 1.1. Introduction

### What is freeze drying (lyophilisation)?

**Freeze drying means:** Removal of water from frozen material. The drying process takes place by direct conversion from ice to vapour. This process is called sublimation. Sublimation happens under vacuum when the temperature in the product is less than -10°C. The aim of freeze drying is to obtain a readily water-soluble product which has the same characteristics as the original product after the addition of water. As the drying process takes place in the frozen state at low temperatures it is possible to dry proteins which will not denature. Most of the other chemical compounds will also remain unchanged. Freeze drying products, of biological origin such as tissues, tissue extracts, bacteria, vaccines and sera transforms them into a dry product. During this process enzymatic, bacterial and chemical changes are largely avoided. Freeze drying is the gentlest process for preserving the biological properties of sensitive tissue and tissue components. Freeze drying can also be used to dry some inorganic products.

## 1.2. Technical data of 100KG freeze driers

<i>Production Freeze Drier Specification</i>	
	<b>100kg</b>
<i>Overall Dimensions W x H x L m</i>	1.6 x 2.25 x 3.2
<i>Drying Chamber Diameter x Length m</i>	1 x 1
<i>Tray Area m² and Levels</i>	10 – 13
<i>Condenser Chamber Temperature</i>	-55 °C
<i>Drying Chamber Temperature Range °C</i>	-50 to +80 °C
<i>Condenser chamber Defrost</i>	Hot Gas
<i>Condenser Ice Capacity</i>	100 litre
<i>Refrigerant</i>	R-507
<i>Vacuum Pump</i>	Pfeiffer Duo 65
<i>Power Requirements</i>	3ph 380 - 415v
<i>Running Power Consumption</i>	20kw
<i>Warranty - Parts and Labour</i>	12 months

## **1.3. Safety instructions**

### **1.3.1. Disconnect the electricity supply before removing panels**

The freeze drier must be securely isolated or unplugged or from the mains supply before the panels are removed or any maintenance work is undertaken.

### **1.3.2. Solvents**

Acidic or high solvent concentration products should not be dried because of corrosion risk and damage to the vacuum pump.

### **1.3.3. Cleaning and Maintenance of the Unit**

For infectious, toxic, pathogenic and radioactive substances, the danger information of the associated safety regulations must be observed.

### **1.3.4. Freezing of skin to surfaces**

Make sure skin does not come into contact with freezing surfaces.

## **1.4. The F100 freeze driers should not be used when:**

1. It is not properly installed.
2. Panels are missing.
3. The operator is not authorized or trained
4. Highly corrosive or solvent substances are present.
5. In hazardous or dangerous locations.
6. The products are explosive or highly flammable.
7. The products are Infectious, toxic, pathogenic or radioactive unless in suitable vessels and in accordance with the relevant safety data.



## 2. Description of the Freeze Drying Processes

### 2.1. General Information on Freeze Drying

Freeze drying is the gentlest process for drying products. It uses the process of sublimation, the direct conversion from solid to vapour state. The frozen product is dried under vacuum without thawing. The condenser chamber works as a cryogenic pump as it takes large volumes of vapour and condenses a small amount of ice. The vacuum pump is only intended to remove the air from the drying chamber but not the vapour.

In order to start the sublimation process, energy must be supplied to the product. This energy source comes from the heated shelves.

Primary drying removes the most of the water from the product.

Secondary drying removes the last traces of water by means of deep vacuum.

The main components of a freeze dryer are:


- Vacuum drying chamber with heated shelves
- Vacuum pump to evacuate air.
- Ice condenser with temperature of  $-55^{\circ}\text{C}$  to condense water vapour.

#### Sublimation


The principle of sublimation is briefly explained using the phase diagram of solid liquid and vapour. If the pressure is higher than 6.1 mbar, water can exist in all three phases (solid, liquid, vapour) when the temperature is lowered or raised. At 6.1 mbar and  $0^{\circ}\text{C}$  all three lines meet, this is called the triple point where all three phase can occur simultaneously. Below this point when the pressure is lower than 6.1 mbar, the ice is converted directly from a solid to a vapour on reaching the sublimation pressure curve.

The sublimation curve shows the vapour pressure of water as affected by temperature and pressure.


Phase diagram for solid, liquid and vapour

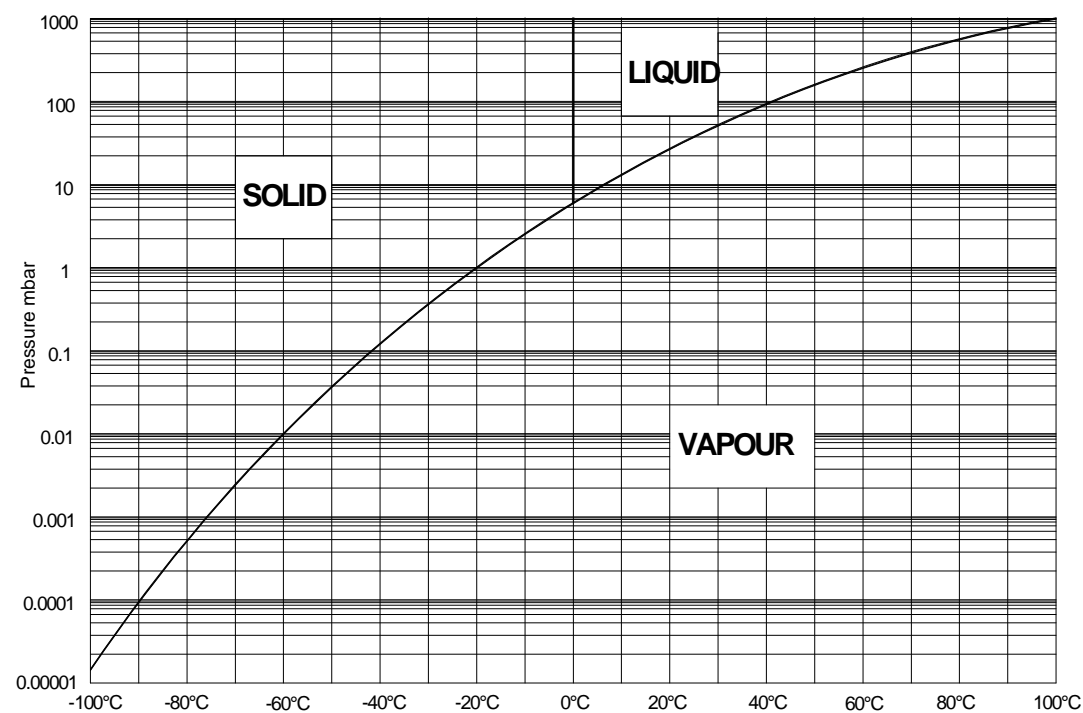


Vapour pressure of ice

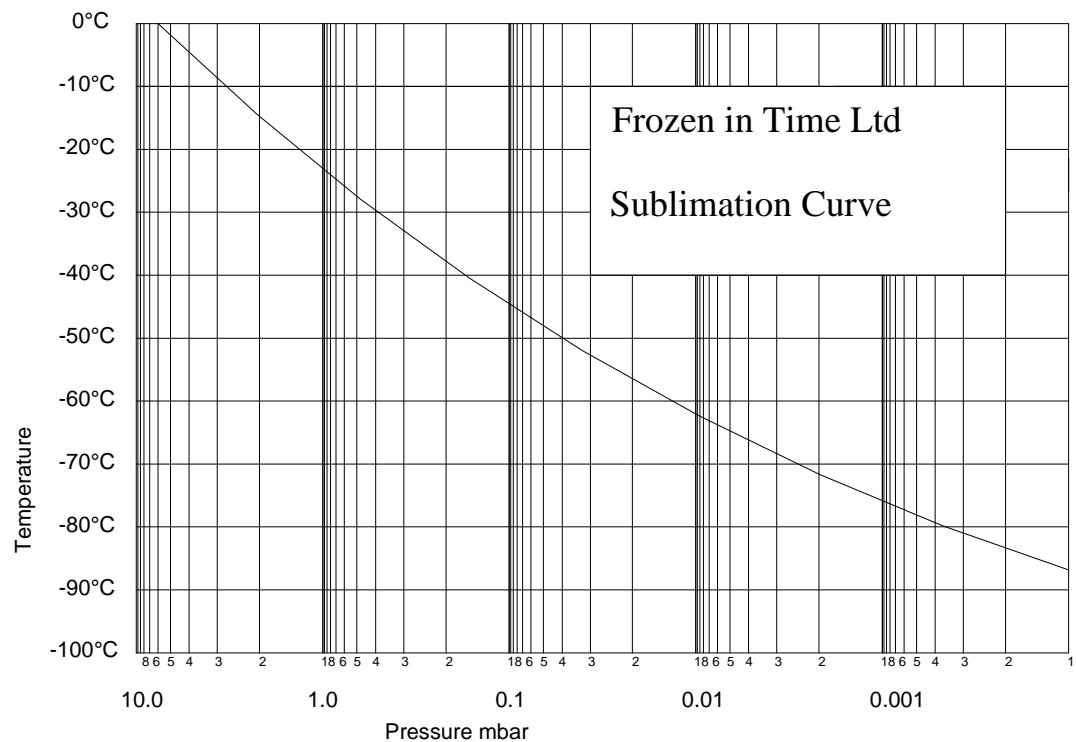

Cross sectional diagram of the freeze driers chambers during **Product freezing** and during **Product drying**.

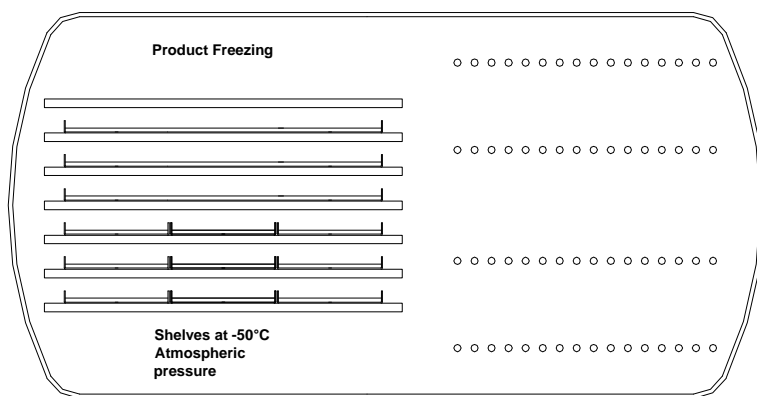

Condenser chamber refrigeration is switched off

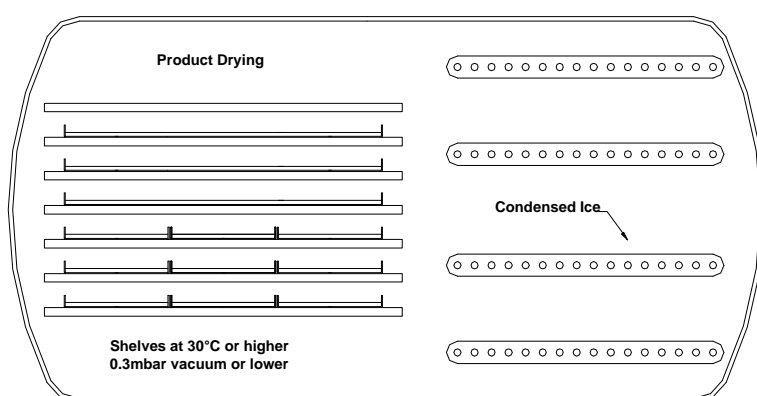

## Product Freezing

The Isolation valve is closed and the product is frozen by the low temperature of the shelves.

## Product drying

The condenser is frozen to its minimum temperature. As the temperature goes below approximately -30°C the vacuum pump can be switched on. The isolation valve must be opened and the vacuum is created in both chambers. When the vacuum is sufficient the heating can be applied to the shelves. Sublimation will cause the products on the shelves to dry. Deposition will occur in the condenser chamber as the sublimated vapour re-freezes.

## 2.2. Freezing the product.

Product can be frozen directly on the shelves of the **F100** freeze drier. This is the usual option for product to be freeze dried in trays or vials. The product is placed on the shelves and the shelves are cooled down to the desired temperature. The freezing can be done in stages, at a controlled rate or just as quickly as possible.

## 2.3. Primary drying

The condenser drops to its operating temperature.

The isolation valve is open

The vacuum pump is switched on.

**The duration of the main drying phase depends mainly on:**

- the layer thickness of the product,
- the solid content of the product,
- the heat supplied to the product during the drying process,
- the vacuum pressure inside the drying chamber during the drying process.

With increasing pressure the rate of sublimation rises as long as it stays below the vapour pressure of the product. This is because at higher pressures the heat energy reaches the sublimation front of the ice core sooner. Therefore the drying period is shortened. The water vapor generated during the main drying phase is not intended to be removed by the vacuum pump. It is to be collected by the ice condenser. The purpose of the vacuum pump is to lower the partial pressure of the non-condensable gases so that the water vapor can be transported from the product to the ice condenser. However, small quantities of water vapor will be removed by the vacuum pump. The vacuum pump is equipped with a gas ballast valve that when open, removes traces of condensable vapors from the pump. For this reason the gas ballast valve can be open during the main primary phase. The gas ballast valve is not required for secondary drying and closing it will help achieve a lower level of vacuum.


During primary drying the moisture is removed by sublimation and during secondary drying the bound moisture is removed by desorption. The recommended vacuum pump should reach with open gas ballast valve, a vacuum level lower than the relevant water vapour pressure.

Shelf temperatures can be raised in stages, at a controlled rate or set to maximum for fastest heat transfer. The heat input must of course not be enough to damage or melt the product. Too much heat will increase the amount of vapours to a point where the vacuum level diminishes to above the eutectic point of the product.

**The residual moisture of the dried product depends mainly on:**

- The temperature of the dried product during the final drying process,
- The final vacuum reached during the final drying process.

The end of the primary drying phase is reached when the product temperature is nearly the same as the shelf temperature (temperature difference between shelf and product approximately 3 to 5°C). Once the primary drying is completed the secondary drying will remove the bound water from the product. The following diagram shows the drying process for a product containing approximately 10 % solid matter. During the first quarter of the primary drying phase approximately 50% of the water content is removed. During the next quarter of the primary drying phase approximately 50% of the remaining water content is removed. This continues until the drying curve approaches the time axis asymptotically. This typical drying curve is due to the fact that the area of sublimation recedes into the product and the remaining water vapour must pass through the already dried layers. During the drying process the resistance increases. The drying curve is determined by the latent heat of sublimation and the amount of vapour transported. In order to increase the specific heat conduction properties of the product and to keep the water vapour volume as low as possible it is necessary that drying takes place as close as possible to the solidification point or eutectic point.

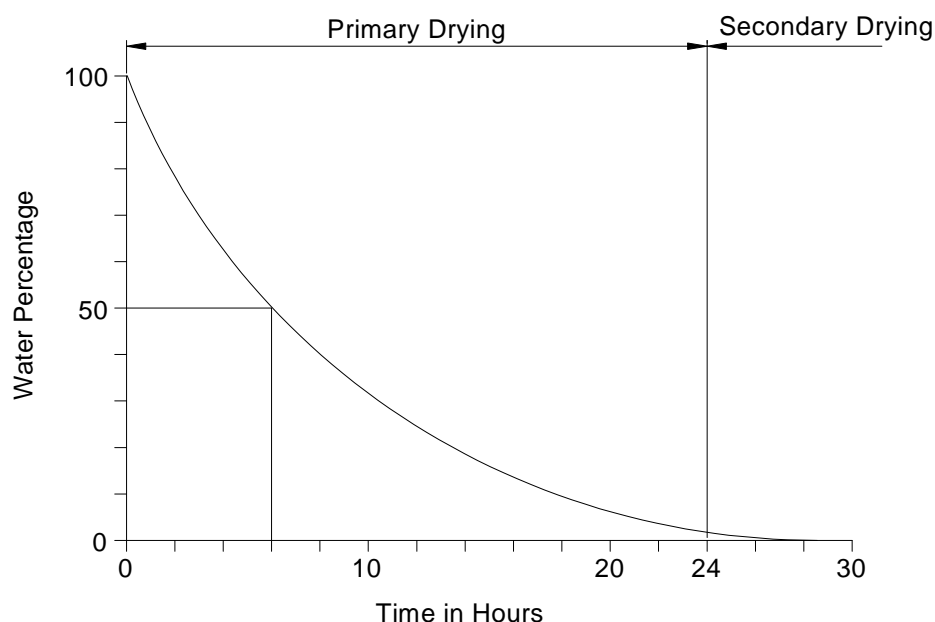

The drying time depends heavily on the vacuum level. The nearer the vacuum to the solidification point in accordance with the vapour pressure curve the shorter the drying time.


### Facts regarding ice in a vacuum:

- 1.0 gram of ice at;
- 1.0 mbar assumes a volume of 1 m<sup>3</sup> vapour
- 0.1 mbar assumes a volume of 10 m<sup>3</sup> vapour
- 0.01 mbar assumes a volume of 100 m<sup>3</sup> vapour

### Heat supply during drying

The required heat supply to the product to be dried takes place by;  
Conduction through contact in the drying chamber  
Mild conduction through low pressure vapour  
Radiant heat energy.

### Affects of freeze drying of a product in a dish

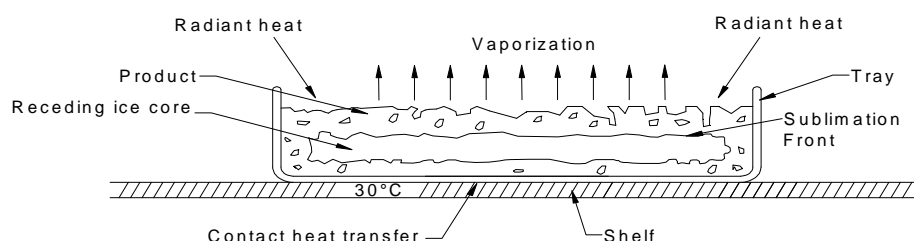

Heat transfer takes place via the heated shelves by direct contact with the bottom of the tray. At the beginning of sublimation the transfer of heat is very effective from the wall of the tray to the frozen product. However, soon an area develops which is ice-free, porous, dried and has an insulating effect between the wall of the tray and the product. This slows down the heat energy transfer available to the ice core. The porous dried layer enables the passage of vapour from the ice core. If it is restricted the temperature will increase and ice core will thaw rather than sublime. This applies especially to inhomogeneous products and to great layer thicknesses. During this drying phase it is important to regulate the heat supply and control temperature and pressure precisely.

## 2.4. Secondary drying

The final pressure in the drying chamber depends on the ice condenser temperature according to the vapor pressure curve above ice:

- e. g. 1.030 mbar correspond to -20°C
- 0.370 mbar correspond to -30°C
- 0.120 mbar correspond to -40°C
- 0.040 mbar correspond to -50°C
- 0.01 mbar correspond to -60°C

The unit is in operating condition if the temperature of the ice condenser is lower than -50°C and the pressure is lower than 0.12 mbar. The final pressure measured when there is no product in the unit and its corresponding ice temperature is determined by the warmest ice surface in the condenser chamber.

## **2.5. Air admittance**

After the vials have been closed the vacuum in the chamber must be released by admitting air. Air will enter through the air admittance valve until the pressure is equalized and the door will release. This may take a few minutes.

## **2.6. Defrosting**

Defrosting of the ice condenser is carried out manually by pressing the defrost button on the manual screen. Defrost time and temperature is adjustable on the engineering screen of the control system. The drain valve must be opened to allow the water/condensate out.

In the automatic program, defrost must be selected from the post program list. Defrost will perform automatically at the end of the process. It will follow the same conditions set on the engineering screen.

## 3. Installation and Commissioning of the 100KG to 1000KG freeze driers.

### 3.1. Site of installation

If the freeze drier is to be situated in a large open area the heat exchangers can remain on the top of the unit. If it is to be in a smaller room then the heat exchangers will need to be fit outside of the enclosed area, preferably externally. In many cases condenser will be water cooled with an external chiller.

### 3.2. Mains power

The operating voltage on the name plate must correspond to the local supply voltage. The 100KG & 250KG freeze driers require a three-phase power supply 380 to 415 Volts.

### 3.3. Drain valve for condensate

The drain valve can be piped to a floor drain or collecting vessel.

### 3.4. Vacuum pump exhaust gases

There is an oil mist filter fitted to the vacuum pump. If the vacuum pump is not filtered oil mist has to be discharged outside. A hose can be connected to the exhaust flange of the vacuum pump that leads into the open air or a vent. During installation of the pipe special care must be taken that condensate cannot flow back into the pump.





## 4. Operating the F100 freeze drier

### 4.1 Loading Trays

Bulk trays can simply slide onto the shelves. Trays can be supplied in various sizes to suit the application. If the freeze drier is configured with several rows of trays then the trays at the rear will be removable with the use of a handle.



## 4.2. Vacuum Pump

The vacuum pump is a two stage Pfeiffer Duo 65  
The Duo65 is a 2 stage rotary vane vacuum pump

There are several interlocks that prevent the vacuum pump from starting in ways that could cause problems.

These include not allowing the pump to start when:

- There is an insufficient temperature in the condenser chamber
- The drain valve is open
- The condenser chamber defrost is switched on
- The Product chamber air admittance valve is open.

In an automatic program the vacuum pump will be controlled completely by the PLC and no user operation is needed or allowed.


The vacuum pump oil should be changed when the pump is warm. The oil level should be visible in the sight glass. The intervals for changing the oil will depend upon the products being freeze dried. The condenser chamber temperature must be lower than the temperature corresponding to the vapour pressure that the product is going to freeze dried at. In the case of water vapour the following is a good guide:

1.030 mbar	correspond to -30°C
0.370 mbar	correspond to -40°C
0.120 mbar	correspond to -50°C
0.040 mbar	correspond to -60°C
0.01 mbar	correspond to -70°C
0.003 mbar	correspond to -80°C

If the product contains large quantities of chemicals that are more volatile than water then lower temperatures in relation to vacuum levels are required.

An oil mist filter should be fitted to the exhaust port of the vacuum pump.

For extra information on the pump please see the separate operating manual.

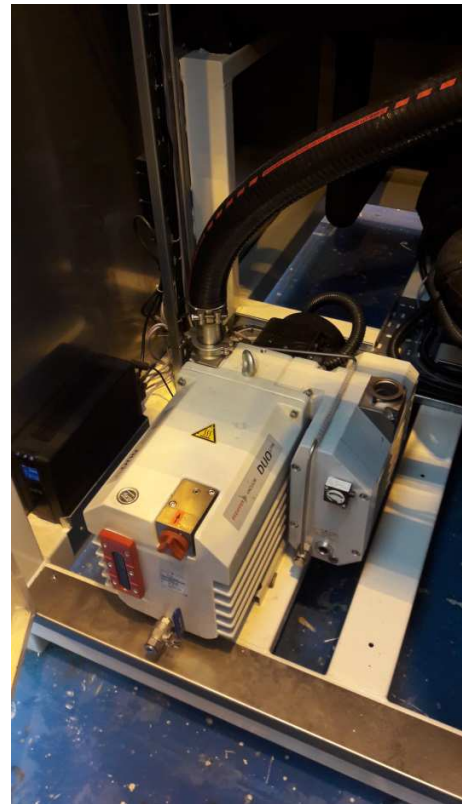

In

## 4.3. Condenser drain valve

As with the Isolation valve and vacuum pump the drain valve can be operated by the controls on the Manual screen. To avoid problems there are two interlocks that prevent the condenser drain valve from being opened when:


- The condenser refrigeration is running
- The vacuum pump is running
- Defrost is running

## 4.4. Circuit breakers

The control box has circuit breakers that may trip out in the event of an electrical problem. If a function is not working, this is the first place to check. There are circuit breakers for the following items.

- PLC
- Control circuit
- Heater
- Circulation pump
- Refrigeration compressor
- Vacuum pump

Please see wiring diagrams for more detailed information

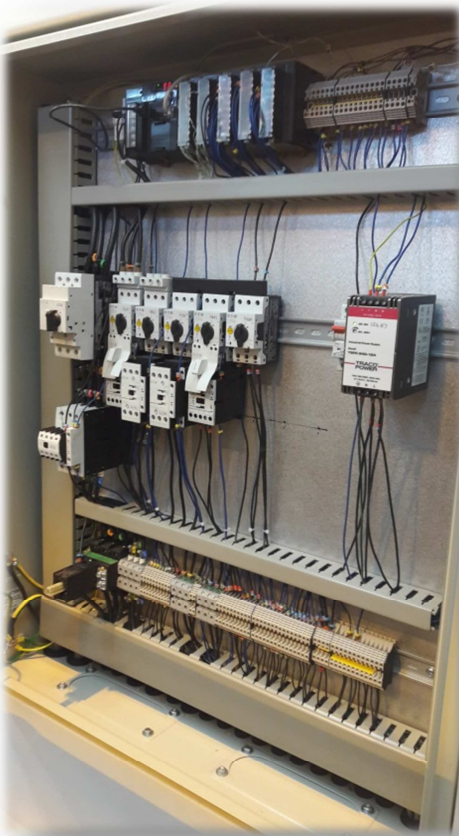

## 5. The control system

The control system for the freeze drier enables the operator to run the freeze drier fully automatically or manually. All data from the drying processes can be logged, saved and printed. The automatic cycles are easily programmed by the operator and can be saved or edited for later use. Programs can be changed while the cycle is running. There is a manual screen for complete manual control. This is often used when trying out a new product before a program is confirmed. The data logging and programming are done on the PC. The running of the program is looked after completely by the PLC. If there is a power failure the computer will safely shut down with the use of a built in uninterruptable power supply.

### 5.1. Manual Control screen

This screen is for manual control. To change to another screen there are selection buttons the down the left hand side.

- Overview
- Manual
- Recipe
- Graph

Next are the function buttons that are used to operate the freeze drier. To the right of each button is the function indicator.

**Pink** means that the function is off but can be activated.

**Green** means that the function is active.

**Red** means that the function is off and cannot be activated due to a current lock on the function. During an automatic run all the manual function buttons are locked.

The function buttons include.

- Shelf Cooling
- Condenser Cooling
- Vacuum Pump
- Drain Valve
- Defrost
- Isolation Valve
- Shelf heating
- Chamber Air inlet

The screenshot displays the 'Manuel' control screen. On the left is a vertical menu with buttons: 'aperçu', 'Manuel' (selected), 'Ingénierie', 'Recette', 'Graphique', 'Minimiser', and 'Fermer'. The main area contains several function buttons with labels and status indicators:

- De** (pink) Refroidissement du plateau
- De** (pink) Condenser Refroidissement
- Désactiver** (red) Pompe à vide
- De** (pink) Vanne de vidange
- De** (pink) Décongeler
- De** (pink) Shelf chauffage
- De** (pink) Chambre Air Inlet

Below these are setpoint fields:

Set Point A sonde	Set Point A Temperature	Set Point B sonde	Set Point B Temperature	Chauffage, pression de vide	Purge manuelle Pression
Etagère 1	40,0 °C	Etagère 1	40,0 °C	1 010,0000 mBar	0,5000 mBar

At the bottom, there are multiple data readout tables:

Sonde	Temp °C	Temp °C	Temp °C	Vac mBar			
Sonde 1	Sensor Err	Etagère	8,1 °C	Condenseur	10,6 °C	Chambre	1 000,0000
Sonde 2	Sensor Err			Interstage	9,6 °C		
Sonde 3	Sensor Err			Cyc Head	10,3 °C		
Sonde 4	Sensor Err			Ref Bar	7,92		
Sonde 5	Sensor Err			Ref Bar	7,91		
Sonde 6	Sensor Err			Ref Bar	7,92		
Moyenne	0,0 °C						

Additional readouts include:

Total	Ref A	Ref kWh
0,00	0,00	0,00

On the right side, there are control buttons: 'Démarrer', 'Auto In Progress', 'Arrêtez', 'Auto en fonctionnement', 'Reinitialiser', 'Auto Complete', and 'pas en fonctionnement'.

Below are the temperature readouts of the shelves or chamber, probes and condenser. There are also vacuum levels in millibars of each chamber.

Set points are required to control temperatures and vacuum levels. If the product is to be lowered in temperature then it will be cooled by the shelf/chamber. There is a thermal lag between the chamber and the product due to the speed of thermal conduction. For fast cooling set the temperature of the chamber lower than the target temperature of the product probe. Once the product probe temperature has reached its set point or the chamber temperature reaches its set point then the cooling will stop. For example;

The chamber temperature is set at -60°C and the probe temperature is set at -40°C.

If the chamber reaches -60°C before the product probe reaches -40°C then the shelf/chamber will hold at -60°C until the product probe reaches -40°C.


If the probe temperature reaches -40°C before the chamber temperature reaches -60°C the product probe will control the shelf temperature.

The same principle applies when heating. The chamber can be set higher to allow the product to heat up quicker.

A further control on chamber heating is vacuum level. If vacuum pressure rises above its set point, heating is deactivated. As sublimation slows down the vacuum level will drop below the set point and heating switches back on.

5.2. Overview screen

Display

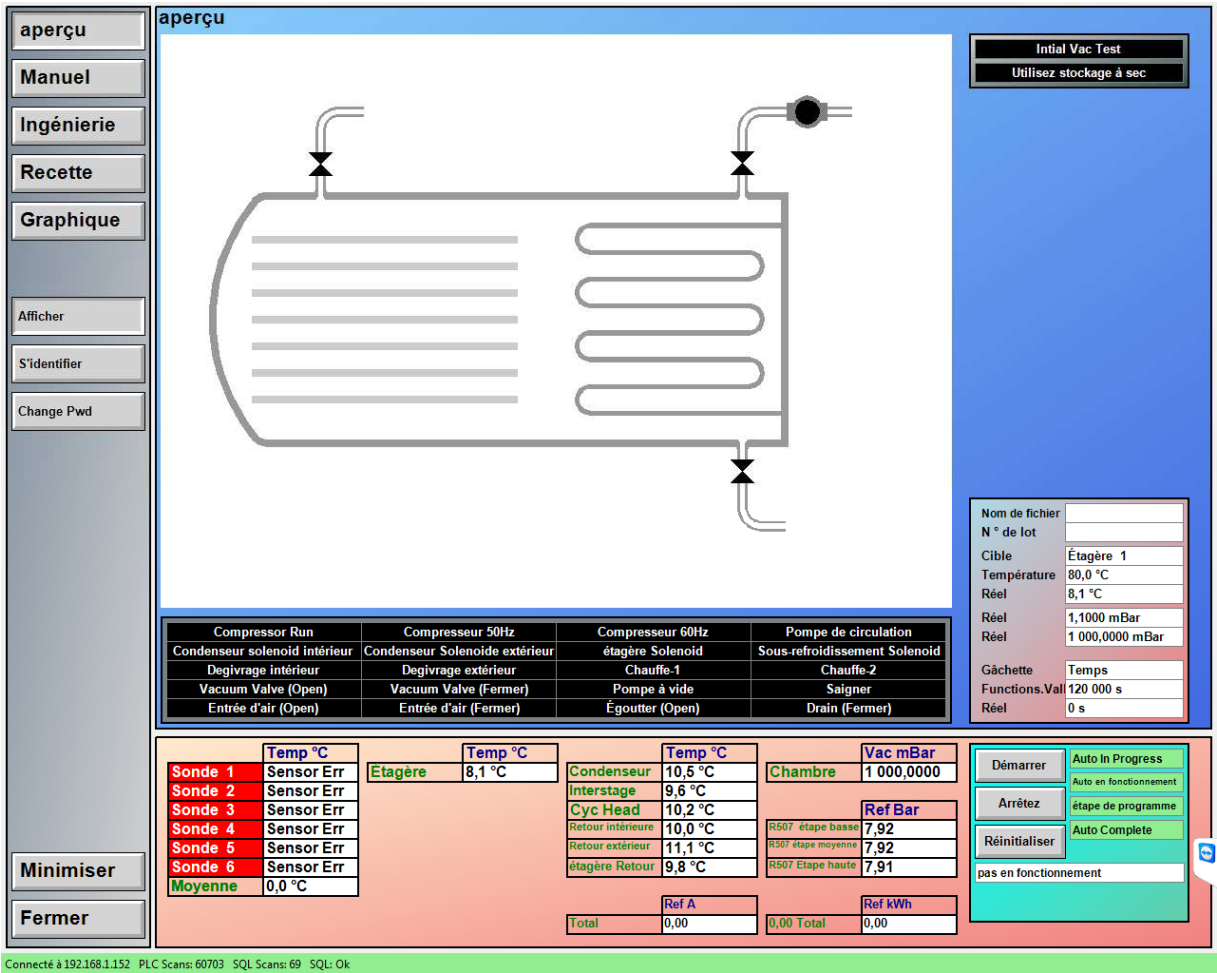

This screen is for is an overview of the freeze drier it shows what parts of the freeze drier are running. Vacuum and temperature set points, program step number and running status are also displayed. The diagram will change depending on what is in operation. In the current view the shelves are red because they are heating. The condenser is blue because it is cooling. The isolation valve between the two chambers is open. Below the picture are black boxes indicating the components of the machine operation. When they are green then that component it active and black indicates that it is inactive.

**Login**

The freeze drier control system has 3 levels of login access. These can be increased upon the customer’s request.


The first level has no access password, it enables the freeze drier operation in manual mode, to load a program/recipe from the list and to start/stop the automated cycle. The user can look through the screens, add and remove lines from the graph and change trace colours.

The second level also allows the programming of recipes, saving and editing. A password is required to access this level


The third level will also give the operator/engineer access to calibration settings and engineering values.A further password is required to access this level.

Whenever a function is not available due to current access level then selection buttons will not be visible.

To log in enter the login name in the first grey box and the login password in the second grey box and then press Login.

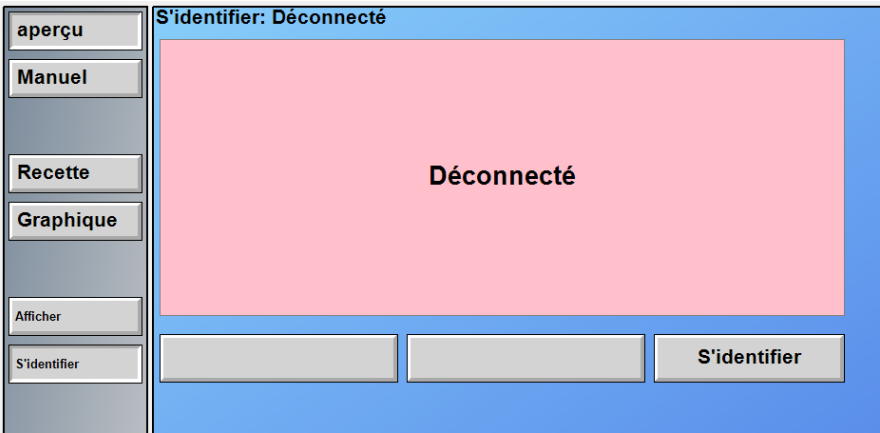

To log out click on the large green rectangle

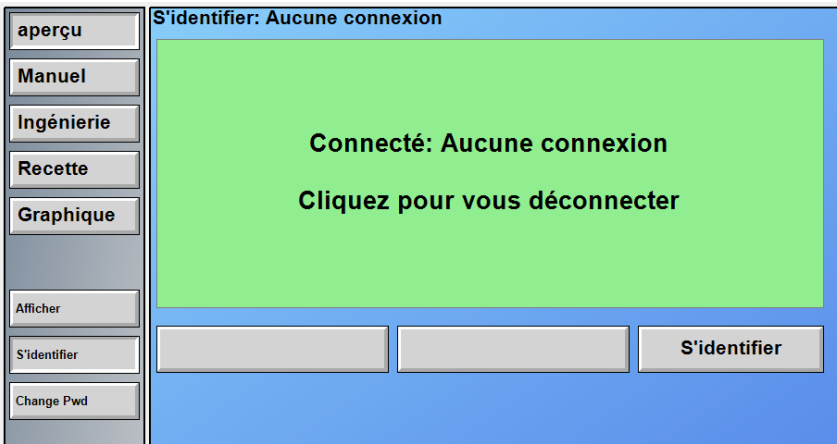



### 5.3. Recipe screen

[illegible]

The Recipe screen is for programming the automatic freeze drying cycle. To change to another screen there are selection buttons down the left side as on previous pages.

There are also options for:

- **Program** - Creating a new programs
- **Options** – Preprogrammed options
- **Load/save** - Save or load a program
- **Receive from PLC** - the details of a program
- **Send to PLC** – the details of a program.
- **Clear** – Clear the programming table

## **Program setup**

The program setup requires the input of a sequence of steps to complete a freeze drying cycle. The operator will define the running conditions within a step and an achievable value to prompt the next step. This value may be a temperature, a vacuum level or a time delay.

When a temperature is entered, the operator will need to specify which temperature probe is to be used.

On this freeze drier the shelves are not temperature controlled, only the chamber.

There are 8 mobile product probes, these are listed:

Probe 1, Probe 2.....

The following is a simplified example of programming a freeze drying cycle to explain the procedure.

## **Entering the first step**

The Shelves are chosen as the target temperature. A triggering condition is set to initiate the next step.

To freeze the product to -40°C the operator could do the following:

The first method

Select the required item such as Chamber temperature at -50°C which would allow the chamber to cool down to this point. As the chamber cools down so will the product. The trigger item would be a product probe 1 set at -40°C. Upon reaching this the next step will be activated. Depending on the type or quantity of product, the thermal lag between the chamber may vary. In the time it takes the product to reach -40°C the chamber may or may not reach -50°C however they will not go below.

The disadvantage of this is:

Setting a minimum chamber temperature gives a constant temperature to absorb heat from the product. As the product temperature gets closer the temperature difference gets less. Therefore the rate of cooling is reduced. Freezing will take longer.

The advantages of this are:

The overall Product temperature will be much more even.

There is less chance of product temperature over shoot.

The chamber does have electrical fans that will operate when cooling if there is not a vacuum present. This will give a more equal temperature throughout the chamber.

The second method

Select the required item as a probe 1 temperature at -40°C. Set the trigger item probe 1 at -40°C. This way the chamber will cool as cold as is possible for the refrigeration system.

The disadvantages of this are:

The overall Product temperature may be much less even.

There is more chance of product temperature over shoot.

The advantage of this is:

Fastest rate of cooling due to greater temperature differences between product and shelf

(Having said this the theory behind this bespoke machine may be proven wrong in practice!!)

## **Entering the second step**

A time step could be used to allow the product to stabilize in temperature. The temperature of the product probe can stay the same so probe 1 is set to -40°C. If the time step was set to one hour, the next step would be triggered after this time.



### **Entering the third step**

The third step could be to create a vacuum on the product.

The temperature of the product would not need further cooling so probe one would remain at -40°C. A vacuum trigger would be selected next with a value of 0.1mbar. The condenser chamber would be automatically cooled to -30°C and the vacuum pump would start.

Once 0.1mbar has been reached the next step would trigger.

As this is the first step that the vacuum is used a value can be put into the target vacuum box. This is the vacuum control setting. This setting will prevent the heater from activating while the vacuum level is above the value entered. As the probe 1 temperature is set at -40°C the system would try and maintain this using heating or cooling. As the vacuum level improves the product will cool by sublimation so the heater would attempt to counter this.

Entering a value into the target vacuum box the same as the trigger value would prevent the heater from activating and allow natural vacuum cooling. The temperature will drop depending upon the level of vacuum created. If the box is left empty or a higher value is entered than the value in the target box then the heater would attempt to maintain probe 1 at the set temperature.

Due to the heat input there will be more sublimation occurring while initial vacuum is being drawn. This will increase the length of time taken to achieve the initial vacuum level.

### **Entering the fourth step**

The fourth step would be to heat the product up to 40°C while maintaining a vacuum level below a set point. This set point is of most importance at the beginning of the primary drying stage when the sublimation rate is at its highest. If the vacuum level rises above a set value then the ice in the product will start to melt. The vacuum control level will ensure that the ice core of the product stays frozen. To achieve the maximum rate of sublimation the vacuum level must correspond to a vapour pressure of a temperature as close to the eutectic point as is safely possible.

With regards to setting the temperatures similar methods as in the first step can be applied. Set a maximum shelf 1 temperature, reducing the chances of over shoot, but expect heat transfer to take longer. Or allow the shelves to heat up to their maximum temperature allowed (settings are in the engineering page) increasing the heat transfer rate, but also increasing the chances of product temperature overshoot.

### **Entering the fifth step**

The fifth step could be a time step to allow the product to stabilize in temperature.

The temperature of the product probe 1 can stay at 40°C. If the time step was set to one hour, the next step would be triggered after this time.

### **Entering the sixth and final step**

The sixth step in this example would be secondary drying. This can be considered as another vacuum step.

The temperature of the product does not need further cooling. Select a trigger item as vacuum, with a value of 0.05mbar. When 0.05mbar is achieved it is the end of the programmable steps. If selected there may be some post steps to complete.

### **Notes:**

Usually programming an automated freeze drying process will involve many more steps detailed steps. As there are several shelves it is sometimes important to repeat each temperature step for each shelf or product probe. This will ensure that every probe reaches the set points required.

## Options

The operator may choose to activate the pre programmed steps listed as

- **Initial Vacuum test**

This ensures that the chambers are going to be vacuum tight before the process is allowed to start. Once the program has started an initial vacuum is pulled on the chambers. As long as a slight vacuum can be reached the program will know that it is safe to start, that the door has not been left open or fittings/seals are missing.

- **Dry storage**

This is a means of storing the product within the freeze drier at a controlled temperature once the process has ended. This is useful if the product finishes its process in the middle of the night and there are no operators to unload it. If products are usually transferred to a fridge after drying then the freeze drier can match these conditions for ideal storage until unloading can take place.



This will open up File Manager. The operator can load a saved Recipe off the list or save one that is currently programmed.

The PLC contains the recipe that the freeze drier will operate with. If the program list has been cleared or programming mistakes have been made then this button will re-populate the programming list with current values on the PLC.

Once a program has been altered, created or loaded then it must be sent to the PLC. This will enable the PLC to operate the freeze drier with the up dated program rather than the last programming it was using.

To delete all program step data off the list and return to a clean unpopulated list press Clear.


<b>aperçu</b> <b>Manuel</b> <b>Ingénierie</b> <b>Recette</b> <b>Graphique</b>  Programme options de Chargement de la sauvegarde  RECV De PLC Envoyer à PLC  Clair Impression	<b>Gestionnaire de fichiers</b>		
	Jam		en haut
			Vers le bas
	Charger la recette	Enregistrer Recette	

[illegible]

## 5.4. Graph

### Show Graph

The data logging monitors temperatures of all mobile probes, shelves, condenser and vacuum levels. Information on temperature and vacuum changes becomes very easy to analyze on a line graph.

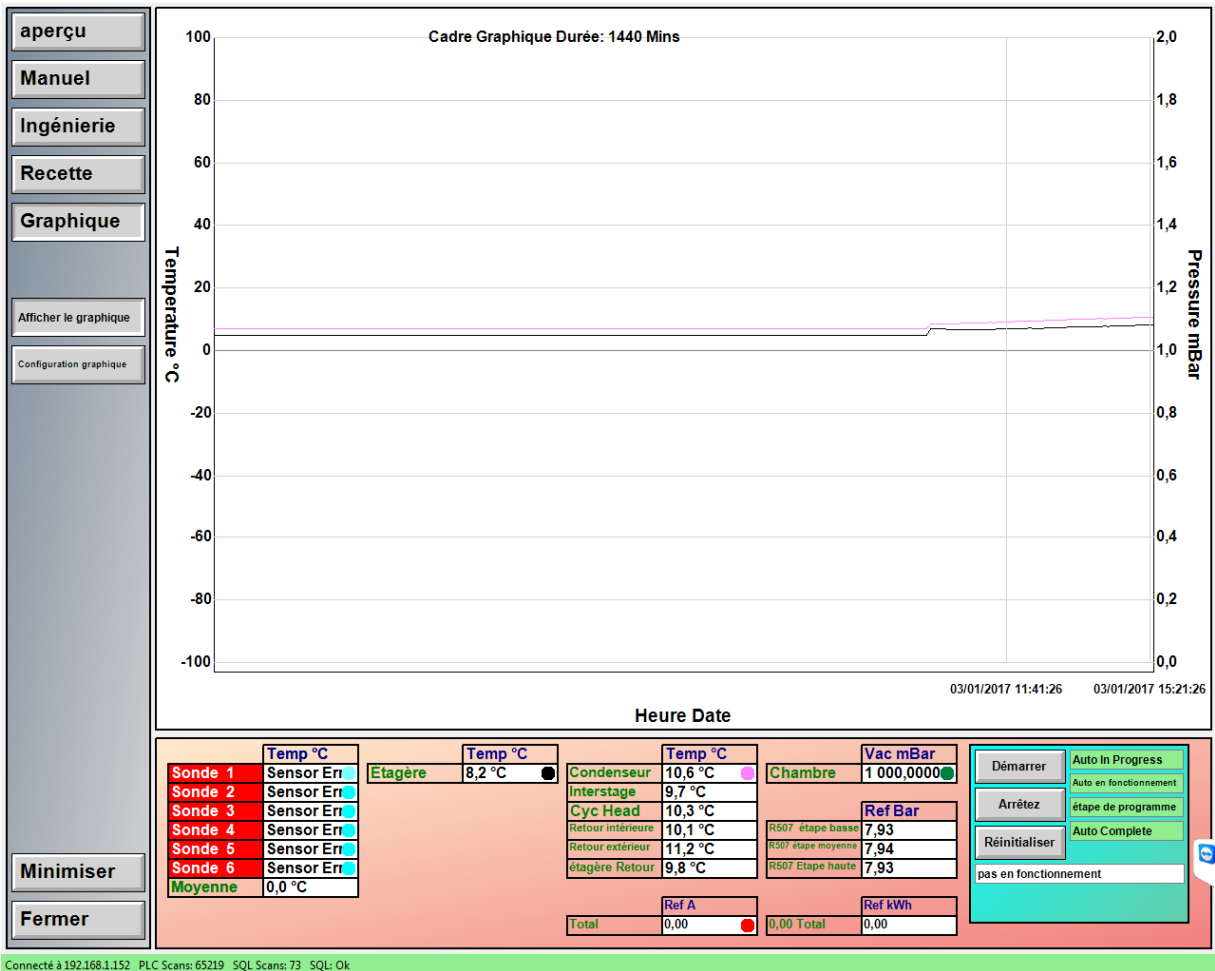

# Graph Setup

aperçu

Manuel

Ingénierie

Recette

Graphique

Afficher le graphique

Configuration graphique

Minimiser

Fermer

Configuration graphique

1440 Mins

5 Mins

30 Mins

1 heures

2 heures

6 heures

12 heures

24 heures

48 heures

96 heures

Affichage de la date

Thermo-couple

Sonde Avg

Sonde 1

Sonde 2

Sonde 3

Sonde 4

Sonde 5

Sonde 6

Shelf 1

Condenseur

Interstage

Cyclinder Head

Retour Intérieure

étagère Retour

Retour extérieur

Graphique

De

Sur

Sur

Sur

Sur

Sur

Sur

De

De

De

De

De

Unité de pression

Chambre de pression

R507 étape basse

R507 étape moyenne

R507 Etape haute

Ampage

Total

kWh

Total

Graphique

De

Sur

De

De

De

Graphique

De

Sur

De

De

Graphique

De

De

	Temp °C		Temp °C		Temp °C		Vac mBar
Sonde 1	Sensor Err	Etagère	8,2 °C	Condenseur	10,7 °C	Chambre	1 000,0000
Sonde 2	Sensor Err			Interstage	9,7 °C		
Sonde 3	Sensor Err			Cyc Head	10,4 °C	Ref Bar	
Sonde 4	Sensor Err			Retour intérieure	10,2 °C	R507 étape basse	7,94
Sonde 5	Sensor Err			Retour extérieur	11,2 °C	R507 étape moyenne	7,94
Sonde 6	Sensor Err			étagère Retour	9,9 °C	R507 Etape haute	7,93
Moyenne	0,0 °C						

	Ref A		Ref kWh
Total	0,00	0,00 Total	0,00

Démarrer

Auto In Progress

Auto en fonctionnement

Arrêtez

étape de programme

Reinitialiser

Auto Complete

pas en fonctionnement

Connecté à 192.168.1.152 PLC Scans: 65337 SQL Scans: 73 SQL: Ok

## Within Graph setup


The time scale that the graph shows can be selected, 30mins to 96 hours. Blue will indicate the time scale that has been selected.

Thermocouple can be identified on the graph by changing the line colour. They can also be hidden by turning them off.

Vacuum pressures can be identified on the graph by changing the line colour. They can also be hidden by turning them off

# The Graph print out

Below is an example of a cycle printout. On the left there is a key to identify graph lines. Product and Batch identification appear as the heading.

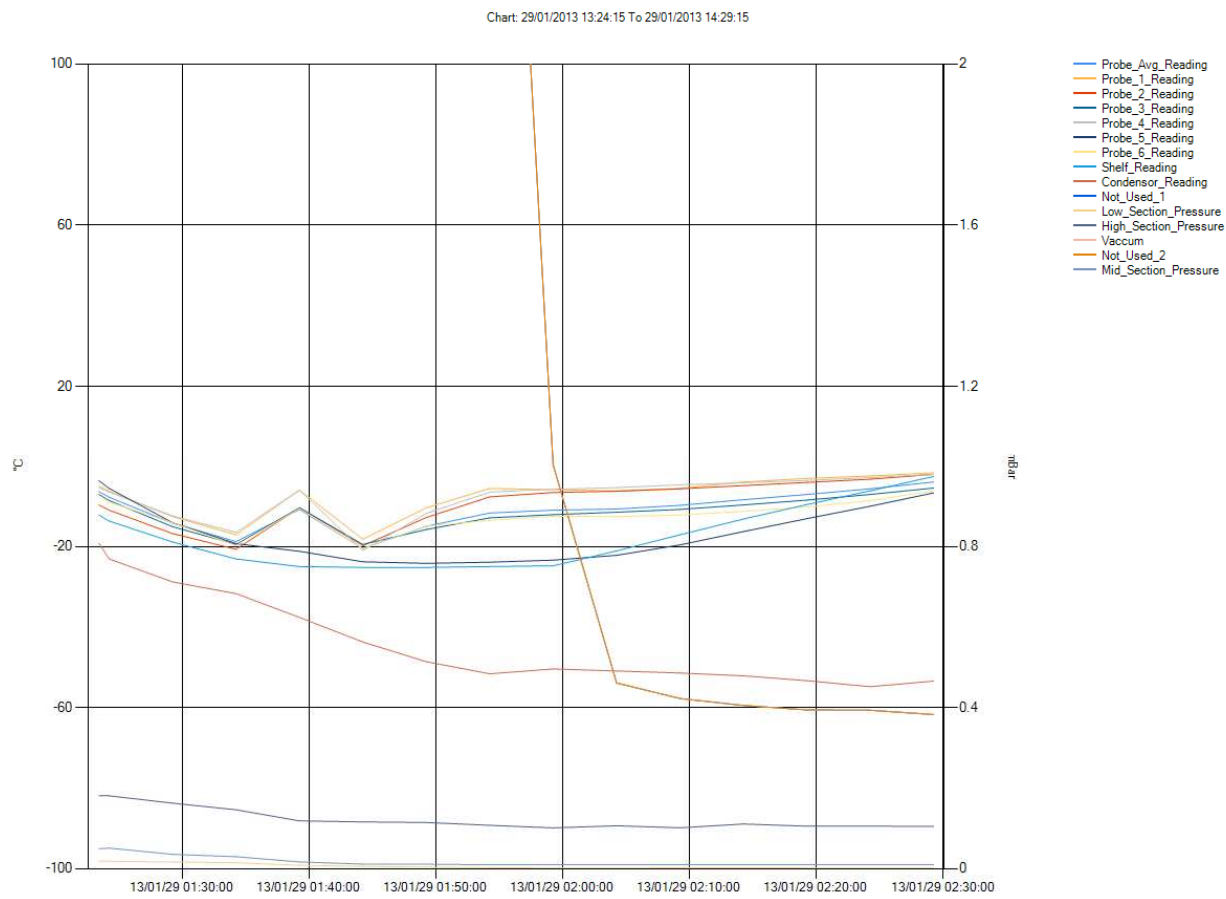

## 5.5. Engineering

The Engineering screen is for programming the automatic freeze drying cycle. To change to another screen there are selection buttons down the left side as on previous pages.

There are also options for:

- **Parameters**—Engineering parameters
- **TC Calibration** – Temperature Calibration
- **Pressure Calibration**—Pressure Calibration
- **Configuration** - configuration

### Engineering Parameters

#### Time allowed For Initial Vacuum Test

This is the time that the vacuum pump will run during an initial vacuum test to confirm the chamber is leak tight before an automated program can start. A moderate vacuum level is set of approximately 600 mbar to confirm doors are closed and the vacuum pump is switched on at the motor. Depending on the volume of the chamber, a sensible time is allowed for this test. As soon as the vacuum level is achieved within the time frame, the test is complete. If the required vacuum is not achieved within the set time the program will not commence. The problem will require investigation.

#### Initial Vacuum Test Pressure

This is the box were the vacuum level is entered. As mentioned above a sensible setting is 600 mbar, this is only achievable with a leak tight vacuum system. This vacuum level will not adversely affect unfrozen product.

#### Max Shelf / Chamber Temperature

A value can be set so that if any temperature goes above it all heating will stop and a warning will be displayed. This is regardless of which sensors are used for temperature control. It is an overall safety limit incase the thermocouple used for temperature control acquires a fault or is poorly programmed or positioned.

#### Max Probe Temperature

A value can be set so that if any temperature goes above it all heating will stop and a warning will be displayed. This is regardless of which sensors are used for temperature control. It is an overall safety limit incase the thermocouple used for temperature control acquires a fault or is poorly programmed or positioned.

#### Vacuum stability Time

The vacuum readings that initiate a change in programmed steps must remain beyond the set point threshold for this selected time. This will ignore sporadic readings on while on the edge of the vacuum sensors designed operating range.

<b>aperçu</b>	<b>Paramètres d'ingénierie</b>	
<b>Manuel</b>	90,0 °C	Température Maximal des étagères / Chambr
<b>Ingénierie</b>	90,0 °C	Max Sonde Température
<b>Recette</b>	0,50 mins	Vacuum Stabilité Temps
<b>Graphique</b>	Étagère 1	Stockage sonde à sec
	4,0 °C	Stockage à sec Température
	60,00 mins	Defrost Période
	50,0 °C	Maximum Defrost Température
	0,50 mins	Refrigeration Turn Off Delay
	0,3 °C	HMI Temp Set Point Hystérésis
	-5,0 °C	Température au démarrage du Vide
Paramètres	5,00 mins	Temps autorisés pour l'essai à vide initial
TC Calibration	600,0000 mBar	La pression initiale d'essai à vide
Calibration de pression	0,5000 mBar	Purge manuelle Pression
Configuration		

**Vacuum start temperature**

This is the temperature set point that does not allow the vacuum pump to start until the condenser temperature is below it. Usually set at -30°C. This will stop unfrozen water vapour being drawn into the vacuum pump.

**Dry product storage probe**

This is the product or shelf probe that is used to control the temperature when the freeze dryer is in dry storage mode. Dry storage can be selected to run after the automated freeze drying cycle has ended if the product is not unloaded straight away. If a cycle ends during the night and the operator cannot unload the freeze drier, preferred conditions such as fridge temperatures can be matched on the shelves. A product or shelf probe may be chosen for this control.

**Dry product storage temperature**

This is the temperature that dry product will be controlled to if dry product storage is selected.

**Defrost time**

This is the time that the condenser chamber will be heated for. A setting that will give enough time to melt all the condensed ice is required. This can be set by the operator to suit the application of the freeze drier.

**Maximum defrost temperature**

This is the maximum temperature that the condenser temperature is allowed to reach while defrosting.

**Refrigeration turn off delay**

The compressors of the refrigeration system will continue to run for a period of time after the refrigeration has been switched off. This will prevent liquid refrigerant being left in areas of pipe work that are exposed to high temperatures.



## Thermocouple Calibration

**aperçu**

**Manuel**

**Ingénierie**

**Recette**

**Graphique**

Paramètres

TC Calibration

Calibration de pression

Configuration

Minimiser

Fermer

### Calibrage de la température

Thermo-couple	statut	Température	Point B Reading	Point B souhaité	Offset	Graphique
Sonde Avg	D'accord	0,0 °C	0,0 °C	0,0 °C	0,0 °C	De
Sonde 1	Sensor Err	0,0 °C	0,0 °C	0,0 °C	0,0 °C	Sur
Sonde 2	Sensor Err	0,0 °C	0,0 °C	0,0 °C	0,0 °C	Sur
Sonde 3	Sensor Err	0,0 °C	0,0 °C	0,0 °C	0,0 °C	Sur
Sonde 4	Sensor Err	0,0 °C	0,0 °C	0,0 °C	0,0 °C	Sur
Sonde 5	Sensor Err	0,0 °C	0,0 °C	0,0 °C	0,0 °C	Sur
Sonde 6	Sensor Err	0,0 °C	0,0 °C	0,0 °C	0,0 °C	Sur
Shelf 1	D'accord	8,2 °C	1,0 °C	1,0 °C	-2,0 °C	De
Condenseur	D'accord	10,6 °C	0,0 °C	0,0 °C	0,0 °C	De
Interstage	D'accord	9,7 °C	0,0 °C	0,0 °C	0,0 °C	De
Cylinder Head	D'accord	10,3 °C	0,0 °C	0,0 °C	0,0 °C	De
Retour Intérieure	D'accord	10,1 °C	0,0 °C	0,0 °C	0,0 °C	De
étagère Retour	D'accord	9,8 °C	0,0 °C	0,0 °C	0,0 °C	De
Retour extérieur	D'accord	11,2 °C	0,0 °C	0,0 °C	0,0 °C	De

	Temp °C
Sonde 1	Sensor Err
Sonde 2	Sensor Err
Sonde 3	Sensor Err
Sonde 4	Sensor Err
Sonde 5	Sensor Err
Sonde 6	Sensor Err
Moyenne	0,0 °C

	Temp °C
Etagère	8,2 °C
Condenseur	10,6 °C
Interstage	9,7 °C
Cyc Head	10,3 °C
Retour intérieure	10,1 °C
Retour extérieur	11,2 °C
étagère Retour	9,8 °C
Total	0,00

	Vac mBar
Chambre	1 000,0000
Ref Bar	
R507 étape basse	7,94
R507 étape moyenne	7,94
R507 Etape haute	7,93
Ref A	
0,00 Total	0,00

Démarrer Auto In Progress

Auto en fonctionnement

Arrêtez étape de programme

Réinitialiser Auto Complete

pas en fonctionnement

Connecté à 192.168.1.152 PLC Scans: 65823 SQL Scans: 73 SQL: Ok

This screen is for factory setup or periodic temperature calibration. Sensor connection status, PLC temperature reading, correction scaling and offset can be set to give the correct reading.

## Vacuum / Pressure Calibration

**aperçu**

**Manuel**

**Ingénierie**

**Recette**

**Graphique**

Paramètres

TC Calibration

Calibration de pression

Configuration

Minimiser

Fermer

### Calibration de pression absolue (Vacuum Calibration)

Unité de pression	Point A mV	Point A Reading	Point B mV	Point B Reading	En train de lire	Couleur
Chambre (basse)	1	1	5000	4000	1 312,2000 mBar	De
Chambre (High)	200	0	8000	8000	1 007,0000 mBar	Sur
R507 étape basse	0	0	800	8000	7,94 Bar	De
R507 étape moyenne	0	0	800	8000	7,94 Bar	De
R507 Etape haute	100	0	3100	8000	7,93 Bar	De

	Temp °C	Temp °C	Temp °C	Vac mBar
Sonde 1	Sensor Err	Etagère 8,2 °C	Condenseur 10,7 °C	Chambre 1 000,0000
Sonde 2	Sensor Err		Interstage 9,7 °C	
Sonde 3	Sensor Err		Cyc Head 10,4 °C	Ref Bar
Sonde 4	Sensor Err		Retour intérieure 10,2 °C	R507 étape basse 7,94
Sonde 5	Sensor Err		Retour extérieur 11,2 °C	R507 étape moyenne 7,94
Sonde 6	Sensor Err		étagère Retour 9,9 °C	R507 Etape haute 7,93
Moyenne	0,0 °C			

	Ref A	Ref kWh
Total	0,00	0,00

Démarrer

Arrêtez

Reinitialiser

pas en fonctionnement

Auto In Progress

Auto en fonctionnement

étape de programme

Auto Complete

Connecté à 192.168.1.152 PLC Scans: 65932 SQL Scans: 73 SQL: Ok

This screen is for factory setup or periodic vacuum calibration. Sensor connection status, PLC Vacuum reading, correction scaling and offset can be set to give the correct reading.

Engineering Configuration

aperçu

Manuel

Ingénierie

Recette

Graphique

Paramètres

TC Calibration

Calibration de pression

Configuration

Minimiser

Fermer

Configuration Ingénierie

De: Mode Diagnostic (Recommander Off)

Sur: Mode avancé (Affichage supplémentaire des données)

De: Mode bureautique (Recommander Off)

Sur: Aucune connexion (Recommander Off)

Sonde 1	Temp °C	Sensor Err
Sonde 2	Temp °C	Sensor Err
Sonde 3	Temp °C	Sensor Err
Sonde 4	Temp °C	Sensor Err
Sonde 5	Temp °C	Sensor Err
Sonde 6	Temp °C	Sensor Err
Moyenne	Temp °C	0,0 °C

Etagère	Temp °C	8,2 °C
---------	---------	--------

Condenseur	Temp °C	10,7 °C
Interstage	Temp °C	9,7 °C
Cyc Head	Temp °C	10,3 °C
Retour intérieure	Temp °C	10,2 °C
Retour extérieur	Temp °C	11,2 °C
étagère Retour	Temp °C	9,9 °C
Total	Ref A	0,00

Chambre	Vac mBar	1 000,0000
	Ref Bar	
R507 étape basse		7,94
R507 étape moyenne		7,94
R507 Etape haute		7,93
	Ref kWh	
0,00 Total		0,00

Démarrer

Auto In Progress

Auto en fonctionnement

Arrêtez

étape de programme

Reinitialiser

Auto Complete

pas en fonctionnement



Connecté à 192.168.1.152 PLC Scans: 66161 SQL Scans: 73 SQL: Ok

Several configurations can be selected, this is for online support of the freeze drier or the software. Extra information can be displayed that would not be needed for the everyday operator. There are several levels/layers of information that displayed. This is only accessible with the higher level of login access.

## 6. Reporting


There is a continual data logging process taking place whenever the freeze drier operating system is in operation. The data logging application is accessible in the windows desktop. Minimize the freeze drier application and open "Reporting".

- 1) Enter the start date and time of the data you wish to view.
- 2) Enter the end date and time.
- 3) If unchecked select "Use Local DB"
- 4) Press "Import Data From Database"

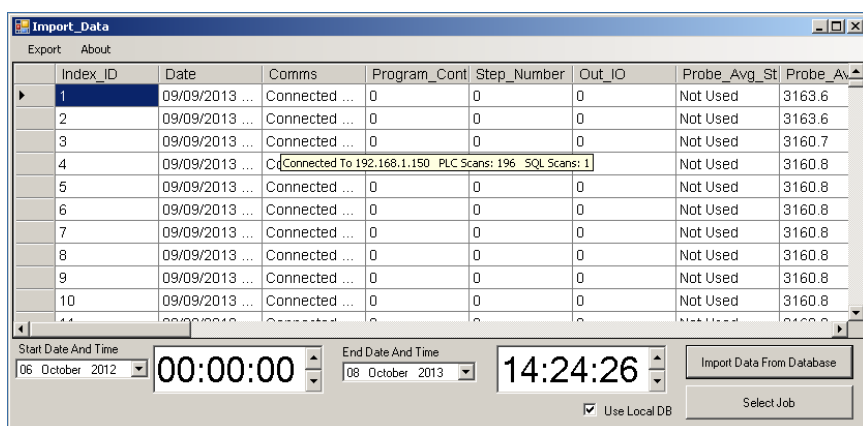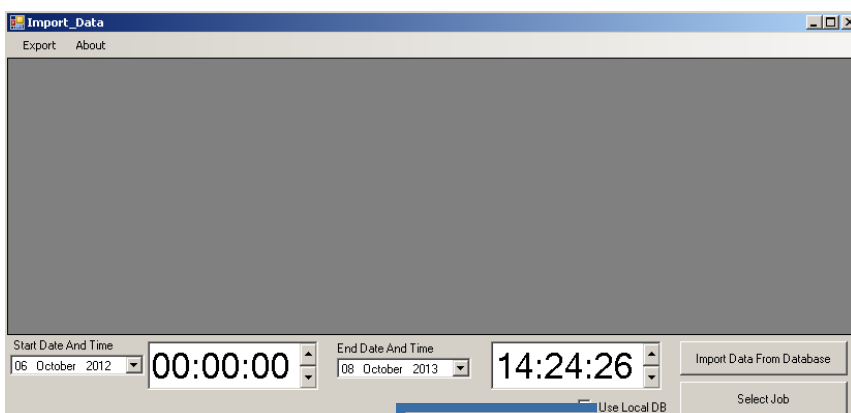

The data base can be scrolled through to find out temperatures vacuum levels and refrigeration pressures for every data logging interval. Each data logging interval is currently set at 1 minute. An extension of this data will show every active function and PLC output.

Select Export send data to CSV, Excel or Graph file.

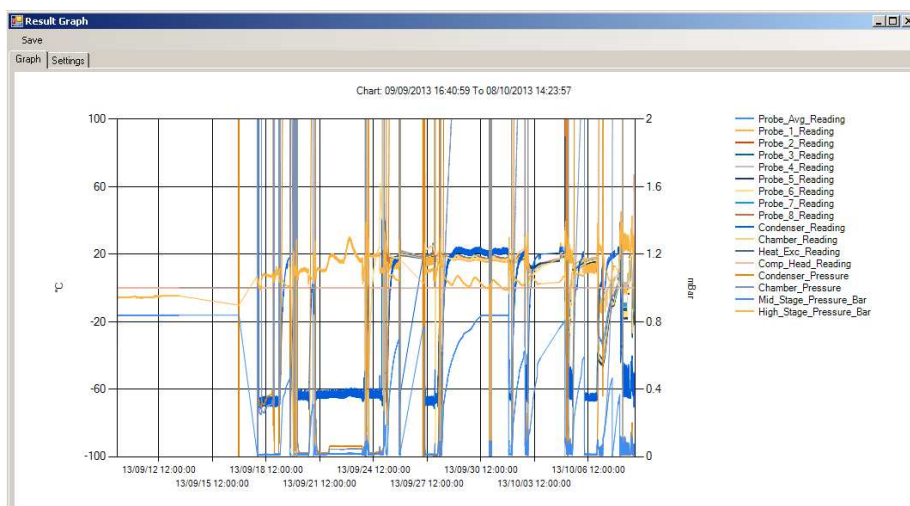

A graph can be generated using the data selected. Trace colours can be changed or removed in the settings page to show the information that important.

# 7. Troubleshooting

## 7.1. Power failure

The freeze drier will resume its program or settings after a power failure. In the event of a power failure in the drying phase, the batch may become unusable. Whether the batch can be saved or not depends on the drying phase in which the product was in when the power failure occurred. If power returns within a few minutes then it is unlikely that any damage will have occurred. It is important to distinguish between the primary drying phase and the secondary drying phase. The product is in the secondary drying phase if the residual moisture has reached approximately 5 %. Below this value, the product is generally not damaged by a power failure.

If the product is in the primary drying phase, it is recommended that the product is refrozen.

It is also advisable to defrost the condenser chamber at this point.

If the product is considered to be still usable then freeze drying can restart.

## 7.2. Insufficient vacuum

Is the vacuum pump is running? If not:

- Check that the pump motor switch is on
- Check that the IEC connection lead is connected
- Check that the vacuum pump circuit breaker has not switched off.
- Check that the contactor is operating.

If the vacuum is sufficient on the condenser chamber but significantly worse on the specimen chamber:

- Check that air admittance and inert gas valves are closed on the overview or manual screen.
- Check all vacuum connections on specimen chamber including door seal. Repair or replace.
- Check for oil leakages from the shelf thermal fluid. Oily residue may collect in the chamber.
- Check for water from cleaning or spilled product residue, this may vaporize preventing vacuum.
- Remove panels and listen for leaks after a vacuum evacuation has been tried.

If the vacuum cannot be achieved in the condenser chamber with the isolation valve closed:

- Check all vacuum connections on condenser chamber including door seal. Repair or replace.
- Check the condition of the isolation valve sealing surface. Glass pieces from broken vials can slit the rubber seal. If there is a doubt about this coat in vacuum pump oil or vacuum grease and test to see if there has been an improvement in the vacuum level.
- Check that there is no suction on the condenser drain hose. This would indicate a leaking valve.
- Check the vacuum pump is pulling an adequate vacuum, test with a separate vacuum sensor.
- Check that the isolation valve is sealing by opening it and pulling a vacuum on the product chamber as well, eliminating the seal of the valve.

If the vacuum pump cannot achieve a sufficient vacuum then replace it or get it repaired.

### 7.3. Insufficient cooling of the condenser chamber

If the condenser chamber is not reaching the relevant temperature -55°C or -85°C  
(Please allow 15% for high load conditions)

- Check to see if there is liquid flow in the refrigeration sight glass. Contact the manufacturer, supplier or a local refrigeration engineer.
- Check the circuit breakers for compressor 1, compressor 2 and fans.
- Check that the contactors are operating.
- Check the overview screen to ensure that refrigeration and condenser cooling are operating.

### 7.4. Insufficient defrosting of the condenser chamber

If defrost is not heating up.

- Check the circuit breaker for defrost
- Check that the contactor is operating.
- Ensure that defrost is activated on the overview screen
- Check that the settings in the Engineering screen are allowing its activation
- Check that temperature control is not controlled by a sensor that is malfunctioning and reading an incorrectly high temperature.

### 7.5. Insufficient cooling of the shelves

If the shelves are not reaching low set points or relevant temperature -45°C or -70°C

- Check to see if there is liquid flow in the refrigeration sight glass. Contact the manufacturer, supplier or a local refrigeration engineer
- Check the circuit breakers for compressor 1, compressor 2, fans and circulation pump
- Check that all the contactors are operating.
- Check the overview screen to ensure that refrigeration, shelf cooling and circulation pump are operating.
- Check that temperature control is not controlled by a sensor that is malfunctioning and reading an incorrectly low temperature.

### 7.6. Insufficient heating of the shelves

If the shelves are not reaching high set points or the relevant temperatures 60°C to 80°C.

- Check the circuit breaker for heater and circulation pump.
- Check that all the contactors are operating.
- Ensure that heater and circulation pump are activated on the overview screen.
- Check that shelf temperature control is not controlled by a sensor that is malfunctioning and reading an incorrectly high temperature.
- Check that there is not an unachievable vacuum set point entered preventing the heater from being activated.
- Check that the settings in the Engineering screen are allowing its activation



## 7.7. Fluctuations in shelf temperatures

If the shelf fluctuations are high it could be due to low levels of thermal fluid in the system. Fluid levels should be topped up when the fluid is at its maximum operating temperature. This is when the level is at its highest it will ensure that no overflowing can occur later. Be sure to reconnect the nitrogen blanketing system after the fluid has been accessed.

Shelf fluctuations occurring when the fluid is below 0°C. This can be caused when water vapour enters the thermal fluid and when it freezes it creates a flow restriction. Please contact the manufacturer, supplier or trained maintenance department. Maintaining a positive nitrogen blanket above the fluid prevents this situation from happening.

Malfunctioning thermocouples can cause sporadic readings or solidly fixed irrelevant readings.

## 7.8. Defrost will not drain away

If the condenser chamber will not drain away after defrost it could be due to a blocked pipe. However first check that the drain valve is opening.

- Check the overview screen to see if the indicator shows that it is activated.
- Check the circuit breaker for the drain valve
- Check that the contactor is operating.
- Check the valve actuator and see if the indicator dial is reading open.
- Check that the manual handle is turning as the valve is activated.

## 7.9. Air admittance will not open

If the vacuum cannot be broken in the product chamber the air admittance valve may not be operating. If it is remove the filter or Nitrogen supply line and try again.

## 7.10. Doors will not seal under vacuum

If the doors will not seal under vacuum

- Check that the vacuum pump is running
- Close the isolation valve and check that the condenser door is sealing
- Check that the air admittance valves are closed
- Clamp the product chamber door and check that it is pushed up against its seal all around.
- Open the isolation valve and release the door clamps.

Does the door still open?

## 7.11. Incorrect probe temperature

Incorrect probe temperatures can be due to

- Unplugged probes
- Broken thermocouples
- Thermocouples with loose connections
- Incorrectly calibrated thermocouples

# 8. Maintenance

## 8.1. Condenser chamber

Before each start-up, ensure that condenser chamber is drained.

## 8.2. Heat exchanger

The refrigeration heat exchanger is used to cool the refrigerant compressed by the refrigeration unit. The heat exchangers are located on each side of the unit and should be kept free of dust or dirt residues. The heat exchanger can be cleaned by brushing, using a vacuum cleaner from the outside or by using compressed air from inside of the unit. Excessive build up on the heat exchanger leads to a decrease in performance and may cause a failure of the unit.

## 8.3. Rubber seals

Special attention must be paid to the rubber seals. If the seals are dirty, they must be removed, cleaned and slightly greased with vacuum grease. If they show signs of cracking they must be replaced.

## 8.4. Vacuum pump

Clean up any oil spills on or around the freeze drier from oil changes.

For the maintenance of the vacuum pump, please refer to the separate operating manual.

Additionally:

The oil level of the vacuum pump must be regularly checked at the sight glass (in case of continuous operation at least once a day). Top up oil to the required level via the oil inlet. Due to possible operation with gas ballast, oil consumption cannot be avoided. For topping-up see the operating manual of the pump. The oil change should always be carried out with warm pump.

## 8.5. Exhaust filter

The exhaust filter should be replaced if it becomes saturated. Where possible there should still be a pipe after the exhaust filter leading into open air. Take care that the condensate in the filter does not rise too high.

## 8.6. Cleaning

### **Cleaning the freeze dryer**

Use soapy water or other water-soluble, mild cleaning agents to clean the freeze dryer. Avoid corrosive and aggressive substances. Do not use alkaline solutions, solvents or agents with abrasive particles. Remove product residues from the ice condenser chamber using a cloth. It is recommended to open the doors of the freeze drier when it is not in use so that moisture can evaporate.

**If there is the risk of toxic, radioactive or pathogenic contamination, special safety measures must be considered and adhered to.**



## 8.7. Checks by the operator

The operator has to ensure the important parts of the freeze dryer and those necessary for safety are not damaged. This especially refers to:

- Doors and hinges
- Seals
- Oil level of vacuum pump
- Heat exchangers
- Exhaust filter