

SMALL CENTRIFUGES

EBA 270

SUPERIOR SEPARATION RESULTS IN MEDICAL APPLICATIONS

The EBA 270 is a small centrifuge with a swing-out rotor that has been developed specifically for use in clinical settings. It can centrifuge the blood tubes and urine tubes up to 15 ml in volume at a maximum speed of 4,000 RPM / 2,254 RCF. Its 90° rotor is ideally suited for spinning blood tubes containing a separating gel.



ROTOR
INCLUDED



HIGHLIGHTS

- max. RPM: 500 - 4,000 min⁻¹
Adjustable in increments of 100
- max. RCF: 2,254
- max. capacity: 6 x 15 ml
- small centrifuge including 6-place swing-out rotor
- compact design
- IVDR-conform according to regulation (EU) 2017/746
- maximum noise level of ≤ 51 dB(A)
- impulse key for short cycle mode
- 2 individual deceleration stages
- easy operation with keypad

FEATURES

- plastic housing
- metal lid
- viewing port in the lid
- one-hand lid lock
- lid dropping protection
- emergency lid lock release
- stainless steel chamber
- brushless drive
- error display
- imbalance switch-off
- backlit panel with actual values of all parameters
- audio message after completion of the centrifugation run


TECHNICAL DATA

EBA 270	
voltage *)	200 – 240 V 1 ~
frequency	50 – 60 Hz
consumption	130 VA
emission, immunity	EN/IEC 61326-1, class B
max. capacity	6 x 15 ml
max. RPM	4,000 min ⁻¹
max. RCF	2,254
running time	1 – 99 min, ∞ continuous run, short cycle mode (impulse button)
dimensions (WxDxH)	326 x 400 x 239 mm
weight	approx. 14 kg
max. noise level	≤ 51 dB (A)
Cat. No.	2300
100 – 127 V 1 ~ / 50–60 Hz	2300-01
consumption	125 VA
emission, immunity	FCC class B

*) Other voltages on request.

AVAILABLE ROTORS

SWING-OUT ROTORS

	angle	max. RPM	max. capacity	Cat. No	page
 swing-out rotor, 6-place	90°	4,000 min ⁻¹	6 x 15 ml	INCLUSIVE	3

SWING-OUT ROTOR, 6-PLACE



Rotor

max. RPM max. RCF	4,000 min ⁻¹ 2,254
max. capacity	6 x 15 ml
run up run down, braked in sec	10 22
angle max. noise level	90° 51 dB (A)
Cat. No.	INCLUSIVE



Vessels

capacity in ml	0.5	0.5	1.5	1.5	2	2	4	5	6	15	1.1 – 1.4	2.6 – 3.4	2.7 – 3	4 – 5.5	4.5 – 5		
Ø x L in mm	10.7 x 46	10.7 x 46	11 x 38	11 x 38	11 x 38	11 x 38	10 x 88	12 x 75	12 x 82	17 x 100	8 x 66	13 x 65	11 x 66	15 x 75	11 x 92		
max. RCF ²⁾	1,359	1,359	1,377	1,377	1,377	1,377	2,254	1,807	1,807	2,254	1,807	1,807	1,807	2,254	2,254		
radius in mm	76	76	77	77	77	77	126	101	101	126	101	101	101	126	126		
Cat. No.	Pediatric		microliter tubes				tubes²⁾				blood collection / urine tubes						

+ 1063-6 + 1063-6 + 1063-6 + 1063-6 + 1063-6 + 1063-6



Adapter

boring Ø x L in mm	17.5 x 80	17.5 x 55	17.5 x 80	17.5 x 55	17.5 x 80	17.5 x 55	17.5 x 80	17.5 x 55	17.5 x 55	17.5 x 80	17.5 x 55	17.5 x 55	17.5 x 55	17.5 x 80	17.5 x 80
vessels per rotor	6	6	6	6	6	6	6	6	6	6	6	6	6	6	6
Cat. No.	2331-6	2333-6	2331-6	2333-6	2331-6	2333-6	2331-6	2333-6	2333-6	2331-6	2333-6	2333-6	2333-6	2331-6	2331-6

Vessels

capacity in ml	4.9	7.5 – 10	10	1.6 – 7	4 – 7	8.5 – 10
Ø x L in mm	13 x 90	15/16 x 92	15 x 102	13/16 x 75	16 x 75	16 x 100
max. RCF ²⁾	2,254	2,254	2,254	1,807	1,807	2,254
radius in mm	126	126	126	101	101	126
Cat. No.	blood collection / urine tubes					



Adapter

boring Ø x L in mm	17.5 x 80	17.5 x 80	17.5 x 80	17.5 x 55	17.5 x 55	17.5 x 80
vessels per rotor	6	6	6	6	6	6
Cat. No.	2331-6	2331-6	2331-6	2333-6	2333-6	2331-6

2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.

CERTIFICATIONS / REGISTRATIONS

Product certification:





Product registration:



Company certifications:



DIMENSIONS – EBA 270

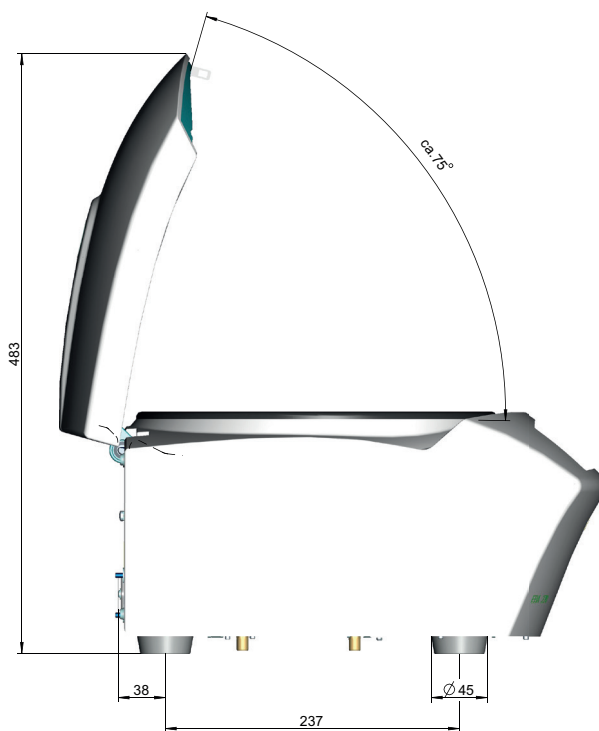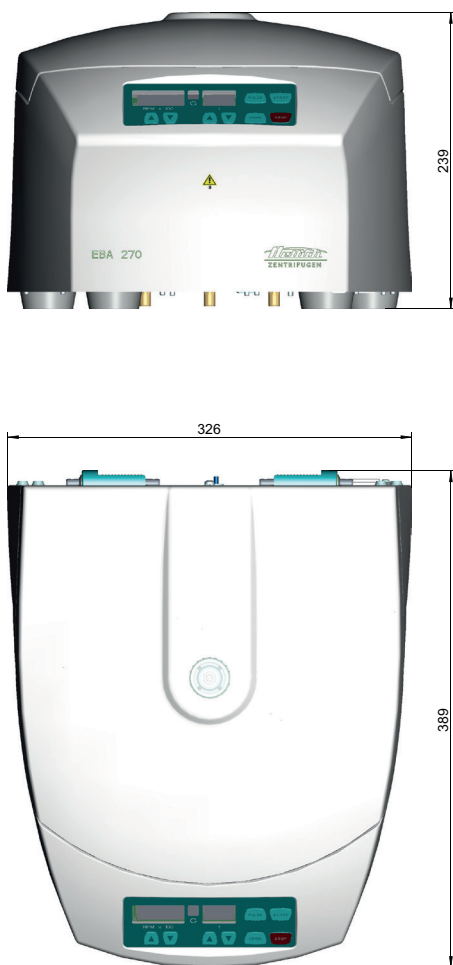



Use the above details to contact us if this literature doesn't answer all your questions.

Pricing on any accessories shown can be found by keying the part number into the search box on our website.

The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed, please provide these to our sales team so that details can be confirmed.

